




**SPECIFICATION**

TEST STANDERD	:	IS 2992 - 1987
ACCURACY	:	= 5 % OVER FIRST EFECTIVE RANGE = 10 % OVER SECOND EFECTIVE RANGE
VOLTAGE	:	= 10 % OF RATED VOLTAGE.
INSYLATION RESISTENCE	:	BETTER THAN 50 MEGOHMS AT 500 VOLTAGE DC
DIE ELECTRIC TEST	:	WITHSTNDS 2 kV AC (rms).
SCALE LENGTH	:	70 mm ( approx.)
WEIGHT	:	650 GRAMS (approx.)
DIEMENSIONS	:	145 x 110 x 70mm ( approx.)
STANDARD ACCESSORIES	:	1. A PAIR OF TESTING LEADS 1 METER IN LENGHTHALONG WITH INSTRUMENT  2. INSTRUCTION BOOKLET  3. TEST CERTIFICATE
OPTIONAL ACCESSORIES	:	1 . A REXINE CARRYING CASE WITH STRAP  2 . A SET OF TEST LEADS 3 METER LONG.

**ILLUSTRATION OF SCALE :**

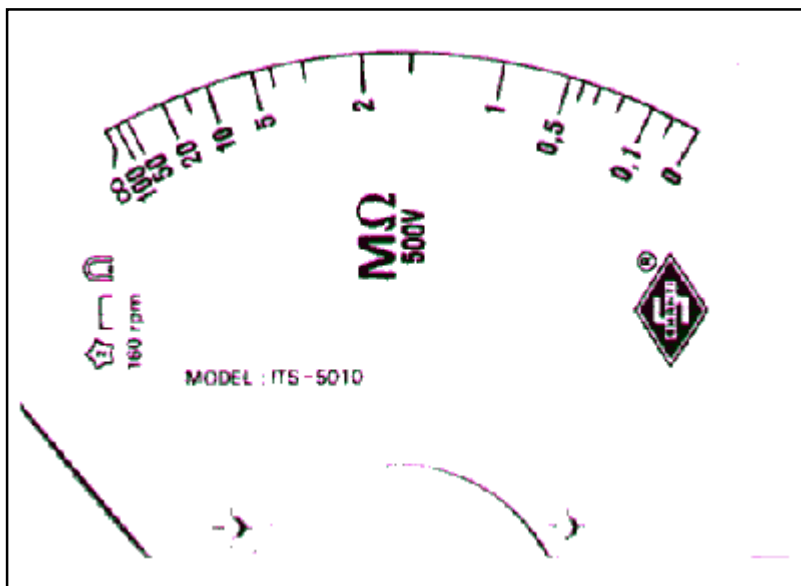

SELECT ANY RANGE FROM THE FOLLOWING :

RATED VOLTAGE	RATED RESISTANCE	MODEL NUMBER
500 V	100 M $\Omega$	ITS - 5010
1000 V	200 M $\Omega$	ITS - 10020

Contact Details :



**Factory Address :**

A-54, MIDC, Andheri (East)  
Mumbai - 400 093  
India

Phone : +91-22-6921426/ 6921425  
Fax : +91-22-8354119  
Email : [shantee@vsnl.com](mailto:shantee@vsnl.com)

**Registered Office :**

A-54, MIDC, Andheri (East)  
Mumbai - 400 093  
India

Phone : +91-22-6921426/ 6921425  
Fax : +91-22-8354119  
Email : [shantee@vsnl.com](mailto:shantee@vsnl.com)

**Visit Us : <http://www.shanti-instruments.com>**